

QUICK SCAN X-RAY DETECTOR

快速扫描X-ray监测仪

Model ~ P 8 Neon Series

型号~P8氖系列

P-8 Neon A ~ P-8 Neon ASC

FEATURES:特点

- DETECTS – ALPHA, BETA, GAMMA, X-RAY
- 探测- α β γ , X-ray
- QUICK SCAN OF LARGE AREAS FOR X-RAY LEAKS
- 快速大面积扫描 X-ray 泄露
- 2" X 16" SENSITIVE AREA
- 敏感面积 2" X 16"
- 8 DETECTORS ON PADDLE
- 带 8 个探测器
- EACH DETECTOR INDIVIDUALLY ALARMED FOR PINPOINTING LEAK
- 每个探测器单独对极细小泄露报警
- USER SETABLE ALARMS
- 用户设定报警
- ALARMS – VISUAL & AUDIO
- 报警-视觉&声音
- SUITCASE MODEL AVAILABLE IN THE P-8 NEON-ASC
- 提供 P-8 NEON-ASC 手提箱型号



APPLICATION 应用

RADIOACTIVE CONTAMINATION ON: 用于辐射污染监测:

- X-RAY SCANNERS X-ray扫描仪
- PACKAGES 包裹
- FLOORS OR WALLS 地板或墙面
-
- State and Federal Regulations require that devices that use or produce X-rays must not emit (leak) X-rays in excess of 0.5 mR/hr from any 10 cm² area as measured at a distance of 5 cm.
- 州和联邦规定X-射线机器辐射泄露每10 cm²区域5cm距离外测量不超过0.5 mR/hr
- This should be verified by complete measurement at time of manufacture, again, upon installation, and periodically thereafter.
- 这一点应该在设备生产、安装及之后定期检查时应该进行核实



TECHNICAL ASSOCIATES
OVERHOFF TECHNOLOGY

Divisions of



US NUCLEAR CORP

7051 Eton Ave., Canoga Park, CA 91303
818-883-7043 (Phone) 818-883-6103 (Fax)

tagold@nwc.net

WWW.TECH-ASSOCIATES.COM

QUICK SCAN X-RAY DETECTOR

快速扫描X-ray监测仪

Model ~ P 8 Neon Series

型号~P8氖系列

P-8 Neon A ~ P-8 Neon ASC

- Specific measurement of alarmed leak area with a small accurate X-ray mR-meter such as Technical Associates' **Model TBM-IC-X-RAY** with 10 cm² active detector area X-Ray compliance adapter is ideal for this task.
- 小巧精确的X-ray mR计量表，如TA公司的型号**Model TBM-IC-X-RAY**，带10 cm²有效探测面积，X-ray符合适配器，理想用于此测量任务。
- Manually scanning the surface of a large cabinet x-ray machine or airport luggage scanner, etc. typically 10 square centimeters at a time is quite tedious.
- 但是如果手动扫描大型X-ray机器机柜或机场行李扫描设备等，一次测量面积典型10平方厘米太苦力了，（所以推荐使用TA公司的**P-8 NEON-A**）

Technical Associates' Quick Sweep Rad Detector **P-8 NEON-A** eliminates such labor intensive scans with large equipment.

TA公司快速扫描辐射监测仪**P-8 NEON-A** 解决了使用大量人力扫描大型设备问题

PROCEDURE: 步骤

1. Pick one side of X-ray cabinet to check first.
选择X-ray机柜一端开始检查
2. Use chalk to divide this side of cabinet into regions or strokes, each 16" wide.
用粉笔将机柜这一端分成几个宽16"区域
3. Set X-Ray emitter to continuous emission or continuous use if possible.
将X-光机设定为连续工作如果有此功能的话
4. Place **P-8 NEON-A** Probe against side of cabinet and sweep it along at about 1 "/second.
将P-8-NEON-A探测器对准机柜外侧以1 "/秒速度扫描
5. Watch the 8 lights on the **P-8 NEON-A** for constant red light.
观察监测仪上的8个红灯是否连续发亮
6. Use the chalk to mark the location of the alarmed light.
用粉笔标出报警灯亮的地方
7. Then continue your sweep.
然后继续扫描
8. When sweeps are completed, come back and repair shielding at the "hot spots" or measure precise mR/hr with TBM-IC-X-Ray.
扫描结束后，返回维修“热点”（泄露）地方的屏蔽或者用TBM-IC-X-Ray精确测量。

SPECIFICATIONS: 规格

- Detector:** Sensitive Area 2" x 16", Window 1.5 - 2.0 mg/cm. Measures Alpha, Beta, Gamma, X-Ray.
探测器: 灵敏面积2" x 16"，窗1.5 - 2.0 mg/cm，测量 α β γ ，X-ray
- ALARM:** 报警
- Locator Lights:** 8 Large Red LED's indicate which of the 8 detectors is firing, i.e. detecting an X-ray leak.
定位灯: 8个LED指示灯中哪个灯亮表示此处X-线泄露



TECHNICAL ASSOCIATES
OVERHOFF TECHNOLOGY

Divisions of



US NUCLEAR CORP

7051 Eton Ave., Canoga Park, CA 91303
818-883-7043 (Phone) 818-883-6103 (Fax)

tagold@nwc.net

WWW.TECH-ASSOCIATES.COM

QUICK SCAN X-RAY DETECTOR

快速扫描X-ray监测仪

Model ~ P 8 Neon Series

型号~P8氖系列

P-8 Neon A ~ P-8 Neon ASC

Audio: Click rate is proportional to radiation level to help locate hottest spots.
Audio emits clicking sound.

声音： 咔嚓音率与辐射水平正比以锁定最热点（泄露）区域

Red light and audio alarm show if total count-rate is above preset users level.
(User settable).

红灯和声音报警显示总计数率是否超过用户预设值（用户设定）

High: Trips at 1 mR/hr- or use recessed adjustment.

高： 触发点1 mR/hr-或使用用户自调


Alert: Trips at 0.1mR/Hr or Adjust.

报警： 触发点0.1mR/Hr或可调整

P-15 probe: Separable 2" dia. Probe with cable and mounting clip. Use for hard to reach corners.

P-15探头： 直径2"可拆卸探头，带缆线和安装卡，用于扫描难以到达的角落

| FEATURES 特点 | P-8 NEON-A |
|-------------------------------|---|
| Alarm levels 报警值 | Alert and high 报警&高限 |
| Alarm Audio 声音报警 | High/low switch 高/低选择 |
| Handles 把手 | Round handle plus metal loops 圆把柄加金属环 |
| Carry Case: (P-8 NEON-ASC 提箱) | Hard sided case, Fitted Foam 硬面箱, 泡沫保护 Handle and shoulder strap 把手和肩带 |

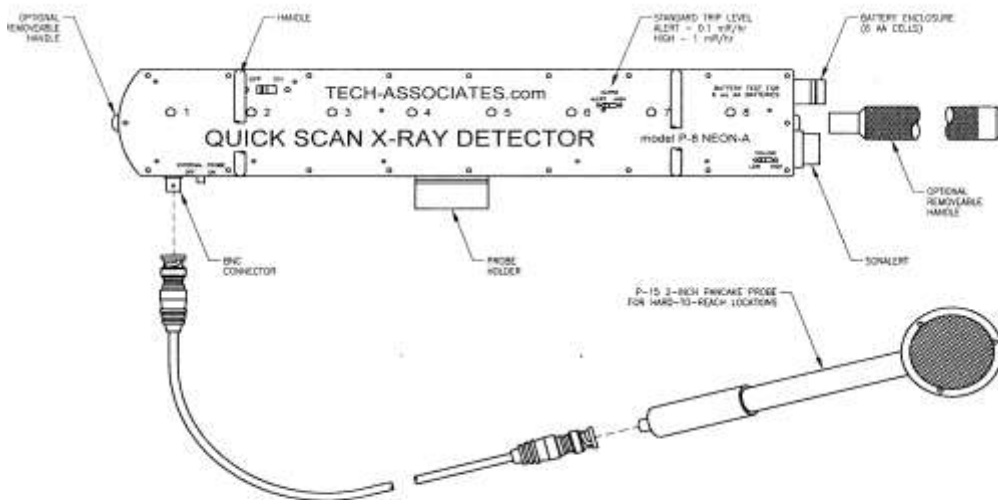

TECHNICAL ASSOCIATES
OVERHOFF TECHNOLOGY

Divisions of



US NUCLEAR CORP

7051 Eton Ave., Canoga Park, CA 91303
818-883-7043 (Phone) 818-883-6103 (Fax)

tagold@nwc.net

WWW.TECH-ASSOCIATES.COM